


PRODUCT DATA SHEET

REFERENCE	DESIGNATION	GTIN CODE
16922	DILATOR PROBE GALL STONE BAKES 13.0 MM 30 CM	3607310004307

VISUAL / DIMENSIONS

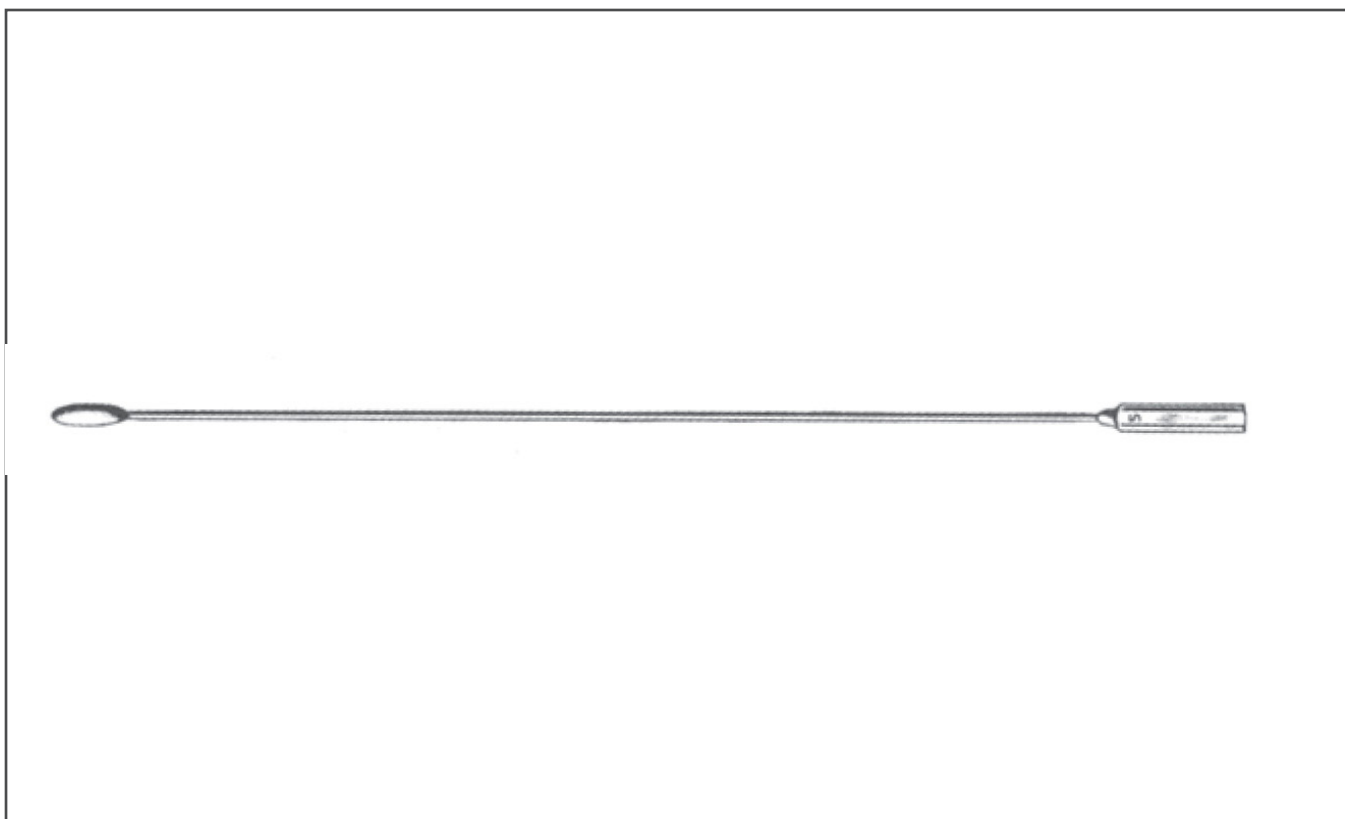

CLASS : IR - NON-STERILE REUSABLE SURGICAL INSTRUMENT

CHARACTERISTICS : SATIN FINISH, LASER MARKING ON THE PLATE.

CLAIMS / SURGICAL SPECIALITY : UROLOGY

MATERIAL / GRADE : MARTENSITIC STAINLESS STEEL : X 20 CR 13

CLEANING / PRE-DISINFECTION : SEE STANDARD OPERATING INSTRUCTIONS.

PACKAGING : WELDED FLEXIBLE BAG WITH PRODUCT LABELLING.